


# The reductions in hypoglycaemia achieved by patients using the FreeStyle Libre system are not at the expense of HbA1c levels<sup>1,2</sup>

Mean HbA1c (change from baseline to 6 months)

## T2DM - REPLACE

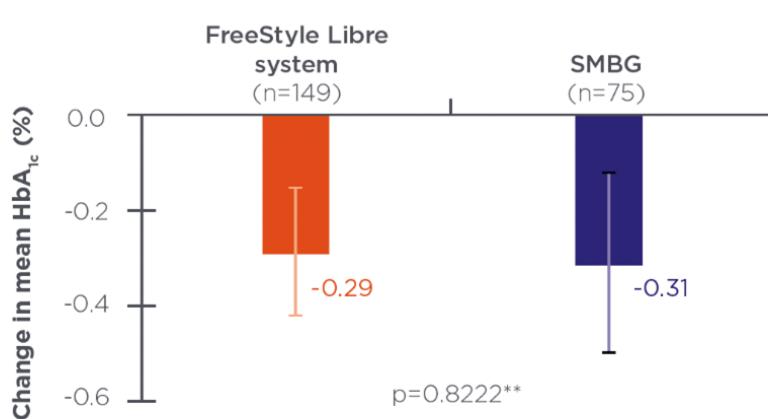


Baseline means:

8.65%

8.75%

## T1DM - IMPACT

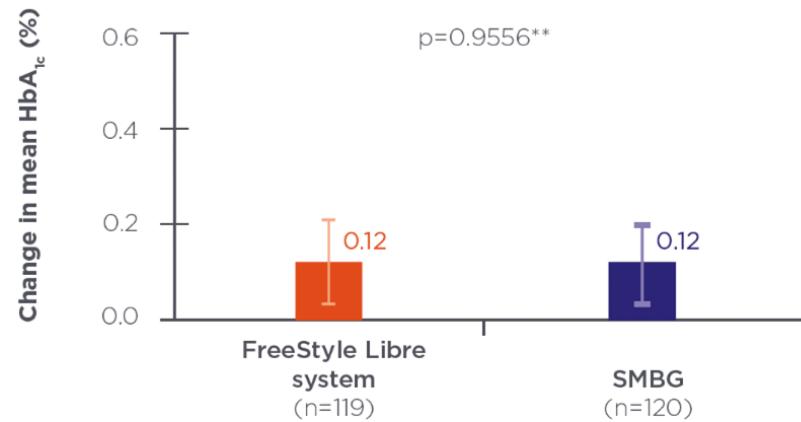

SMBG = self-monitoring of blood glucose; T1DM = type 1 diabetes mellitus; T2DM = type 2 diabetes mellitus

\*\* Adjusted difference versus SMBG.

1. Haak T, Hanaire H, Aijan R, Hermanns N, Riveline JP, Rayman G. Flash Glucose-Sensing Technology as a Replacement for Blood Glucose Monitoring for the Management of Insulin-Treated Type 2 Diabetes: a Multicenter, Open-Label Randomized Controlled Trial. *Diabetes Ther.* 2017 Feb;8(1):55-73. doi: 10.1007/s13300-016-0223-6.

2. Bolinder J, Antuna R, Geelhoed-Duijvestijn P, Kroger J, Weitgasser R. Novel glucose-sensing technology and hypoglycaemia in type 1 diabetes: a multicentre, non-masked, randomised controlled trial [published online September 12, 2016]. *Lancet.* 2016; [http://dx.doi.org/10.1016/S0140-6736\(16\)31535-5](http://dx.doi.org/10.1016/S0140-6736(16)31535-5)